

Nano-Hexapod on the micro-station

Dehaeze Thomas

November 15, 2024

Contents

1	Short Stroke Metrology System	4
1.1	Metrology Kinematics	5
1.2	Rough alignment of the reference spheres	6
1.3	Tip-Tilt adjustment of the interferometers	6
1.4	Fine Alignment of reference spheres using interferometers	6
1.5	Estimated measurement volume	7
1.6	Estimated measurement errors	7
2	Identified Open Loop Plant	10
2.1	First Open-Loop Plant Identification	10
2.2	Better Angular Alignment	11
2.3	Open-Loop Identification after alignment	12
2.4	Effect of Payload Mass	13
2.5	Effect of Spindle Rotation	13
2.6	Identification of Spurious modes	13
3	Decentralized Integral Force Feedback	16
3.1	IFF Plant	16
3.2	IFF Controller	16
3.3	Estimated Damped Plant	19
4	High Authority Control in the frame of the struts	20
4.1	Damped Plant	20
4.2	Robust Controller Design	22
4.3	Estimation of performances	22
4.4	Robustness to change of payload	24
	Bibliography	26


Now that the nano-hexapod is mounted and that a good multi-body model of the nano-hexapod The system is validated on the ID31 beamline.

At the beginning of the project, it was planned to develop a long stroke 5-DoF metrology system to measure the pose of the sample with respect to the granite. The development of such system was complex, and was not completed at the time of the experimental tests on ID31. To still validate the developed nano active platform and the associated instrumentation and control architecture, a 5-DoF short stroke metrology system was developed (Section 1).


The identify dynamics of the nano-hexapod fixed on top of the micro-station was identified for different experimental conditions (payload masses, rotational velocities) and compared with the model (Section 2).

Decentralized Integral Force Feedback is then applied to actively damp the plant in a robust way (Section 3).

High authority control is then applied (Section 4).

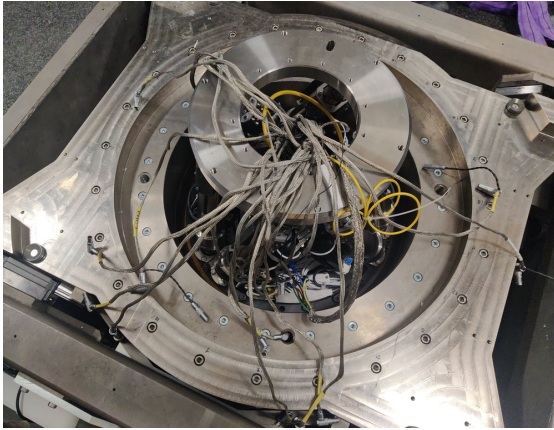

(a) Micro-station and nano-hexapod cables

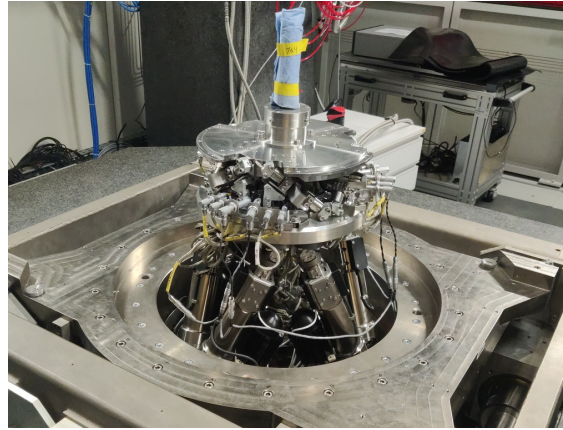

(b) Nano-hexapod fixed on top of the micro-station

Figure 1: Picture of the micro-station without the nano-hexapod (a) and with the nano-hexapod (b)

1 Short Stroke Metrology System

The control of the nano-hexapod requires an external metrology system measuring the relative position of the nano-hexapod top platform with respect to the granite. As the long-stroke ($\approx 1\text{ cm}^3$) metrology system was not developed yet, a stroke stroke ($> 100\ \mu\text{m}^3$) was used instead to validate the nano-hexapod control.

A first considered option was to use the “Spindle error analyzer” shown in Figure 1.1a. This system comprises 5 capacitive sensors which are facing two reference spheres. As the gap between the capacitive sensors and the spheres is very small¹, the risk of damaging the spheres and the capacitive sensors is high.

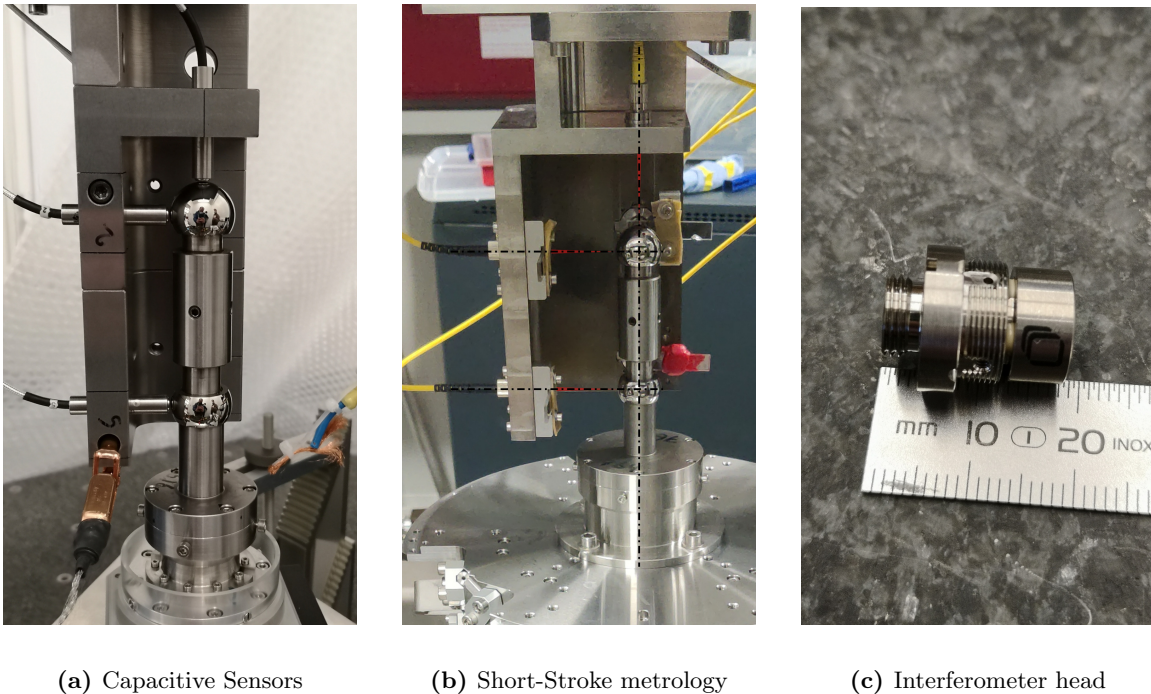


Figure 1.1: Short stroke metrology system used to measure the sample position with respect to the granite in 5DoF. The system is based on a “Spindle error analyzer” (a), but the capacitive sensors are replaced with fibered interferometers (b). Interferometer heads are shown in (c)

Instead of using capacitive sensors, 5 fibered interferometers were used in a similar way (Figure 1.1b). At the end of each fiber, a sensor head² (Figure 1.1c) is used, which consists of a lens precisely positioned with respect to the fiber’s end. The lens is focusing the light on the surface of the sphere, such that it

¹Depending on the measuring range, gap can range from $\approx 1\ \mu\text{m}$ to $\approx 100\ \mu\text{m}$

²M12/F40 model from Attocube

comes back to the fiber and produces an interference. This way, the gap between the sensor and the reference sphere is much larger (here around 40 mm), removing the risk of collision.

Nevertheless, the metrology system still has limited measurement range, as when the spheres are moving perpendicularly to the beam axis, the reflected light does not coincide with the incident light, and for some perpendicular displacement, the interference is too small to be detected.

1.1 Metrology Kinematics

The developed short-stroke metrology system is schematically shown in Figure 1.2. The point of interest is indicated by the blue frame $\{B\}$, which is located $H = 150\text{ mm}$ above the nano-hexapod's top platform. The spheres have a diameter $d = 25.4\text{ mm}$, and indicated dimensions are $l_1 = 60\text{ mm}$ and $l_2 = 16.2\text{ mm}$. In order to compute the pose of the $\{B\}$ frame with respect to the granite (i.e. with respect to the fixed interferometer heads), the measured small displacements $[d_1, d_2, d_3, d_4, d_5]$ by the interferometers are first written as a function of the small linear and angular motion of the $\{B\}$ frame $[D_x, D_y, D_z, R_x, R_y]$ (1.1).

$$d_1 = D_y - l_2 R_x, \quad d_2 = D_y + l_1 R_x, \quad d_3 = -D_x - l_2 R_y, \quad d_4 = -D_x + l_1 R_y, \quad d_5 = -D_z \quad (1.1)$$

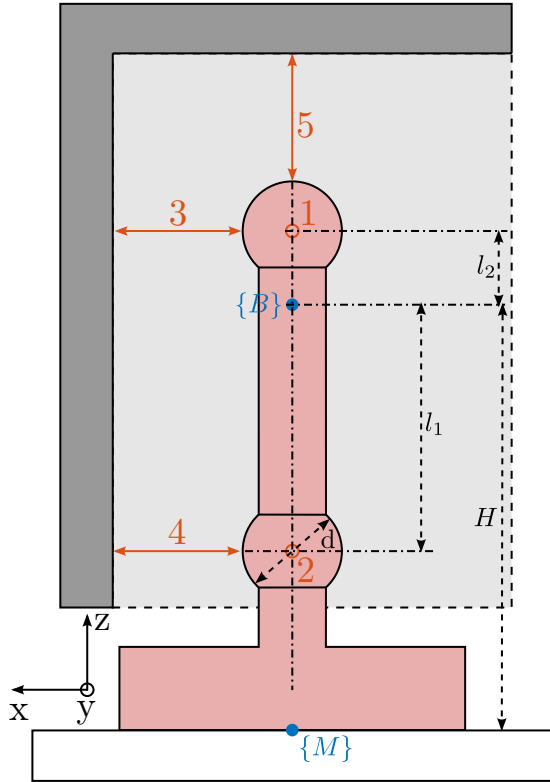


Figure 1.2: Schematic of the measurement system. Measured distances are indicated by red arrows.

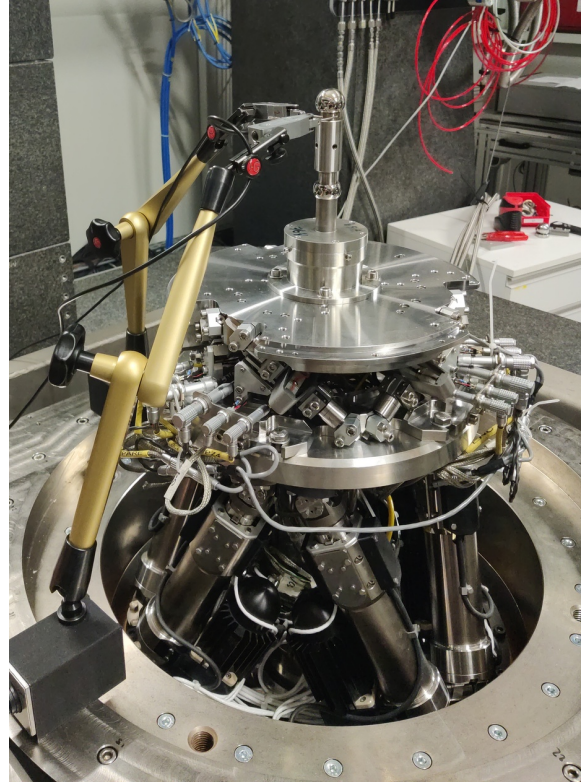


Figure 1.3: The top sphere is aligned with the rotation axis of the spindle using two probes.

The five equations (1.1) can be written in a matrix form, and then inverted to have the pose of $\{B\}$ frame as a linear combination of the measured five distances by the interferometers (1.2).

$$\begin{bmatrix} D_x \\ D_y \\ D_z \\ R_x \\ R_y \end{bmatrix} = \begin{bmatrix} 0 & 1 & 0 & -l_2 & 0 \\ 0 & 1 & 0 & l_1 & 0 \\ -1 & 0 & 0 & 0 & -l_2 \\ -1 & 0 & 0 & 0 & l_1 \\ 0 & 0 & -1 & 0 & 0 \end{bmatrix}^{-1} \cdot \begin{bmatrix} d_1 \\ d_2 \\ d_3 \\ d_4 \\ d_5 \end{bmatrix} \quad (1.2)$$

1.2 Rough alignment of the reference spheres

The two reference spheres are aligned with the rotation axis of the spindle. To do so, two measuring probes are used as shown in Figure 1.3.

To not damage the sensitive sphere surface, the probes are instead positioned on the cylinder on which the sphere is mounted. First, the probes are fixed to the bottom (fixed) cylinder to align its axis with the spindle axis. Then, the probes are fixed to the top (adjustable) cylinder, and the same alignment is performed.

With this setup, the precision of the alignment of both sphere better with the spindle axis is expected to be limited to $\approx 10 \mu m$. This is probably limited due to the poor coaxiality between the cylinders and the spheres. However, the alignment precision should be enough to stay in the acceptance of the interferometers.

1.3 Tip-Tilt adjustment of the interferometers

The short stroke metrology system is placed on top of the main granite using a gantry made of granite blocs to have good vibration and thermal stability (Figure 1.4).

The interferometers need to be aligned with respect to the two reference spheres to approach as much as possible the ideal case shown in Figure 1.2. The vertical position of the spheres is adjusted using the micro-hexapod to match the height of the interferometers. Then, the horizontal position of the gantry is adjusted such that the coupling efficiency (i.e. the intensity of the light reflected back in the fiber) of the top interferometer is maximized. This is equivalent as to optimize the perpendicularity between the interferometer beam and the sphere surface (i.e. the concentricity between the beam and the sphere center).

The lateral sensor heads (i.e. all except the top one), which are each fixed to a custom tip-tilt adjustment mechanism, are individually oriented such that the coupling efficient is maximized.

1.4 Fine Alignment of reference spheres using interferometers

Thanks to the good alignment of the two reference spheres with the spindle axis and to the fine adjustment of the interferometers orientations, the interferometer measurement is made possible during

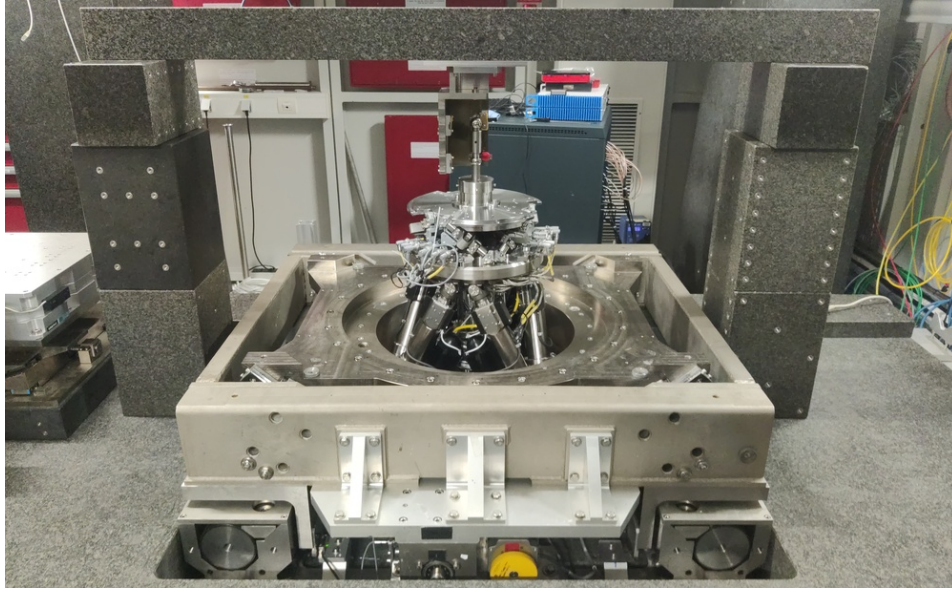


Figure 1.4: Granite gantry used to fix the short-stroke metrology system

complete spindle rotation. This metrology and therefore be used to better align the axis defined by the two spheres' center with the spindle axis.

The alignment process is made by few iterations. First, the spindle is scanned and the alignment errors are recorded. From the errors, the motion of the micro-hexapod to better align the spheres is determined and the micro-hexapod is moved. Then, the spindle is scanned again, and the new alignment errors are recorded.

This iterative process is first perform for angular errors (Figure 1.5a) and then for lateral errors (Figure 1.5b). Remaining error after alignment is in the order of $\pm 5 \mu\text{rad}$ for angular errors, $\pm 1 \mu\text{m}$ laterally and less than $0.1 \mu\text{m}$ vertically.

1.5 Estimated measurement volume

Because the interferometers are pointing to spheres and not flat surfaces, the lateral acceptance is limited. In order to estimate the metrology acceptance, the micro-hexapod is used to perform three accurate scans of $\pm 1 \text{ mm}$, respectively along the the x , y and z axes. During these scans, the 5 interferometers are recorded, and the ranges in which each interferometer has enough coupling efficiency for measurement are estimated. Results are summarized in Table 1.1. The obtained lateral acceptance for pure displacements in any direction is estimated to be around $+/- 0.5 \text{ mm}$, which is enough for the current application as it is well above the micro-station errors to be actively corrected.

1.6 Estimated measurement errors

When using the NASS, the accuracy of the sample's positioning is linked to the accuracy of the external metrology. However, to validate the nano-hexapod with the associated instrumentation and control

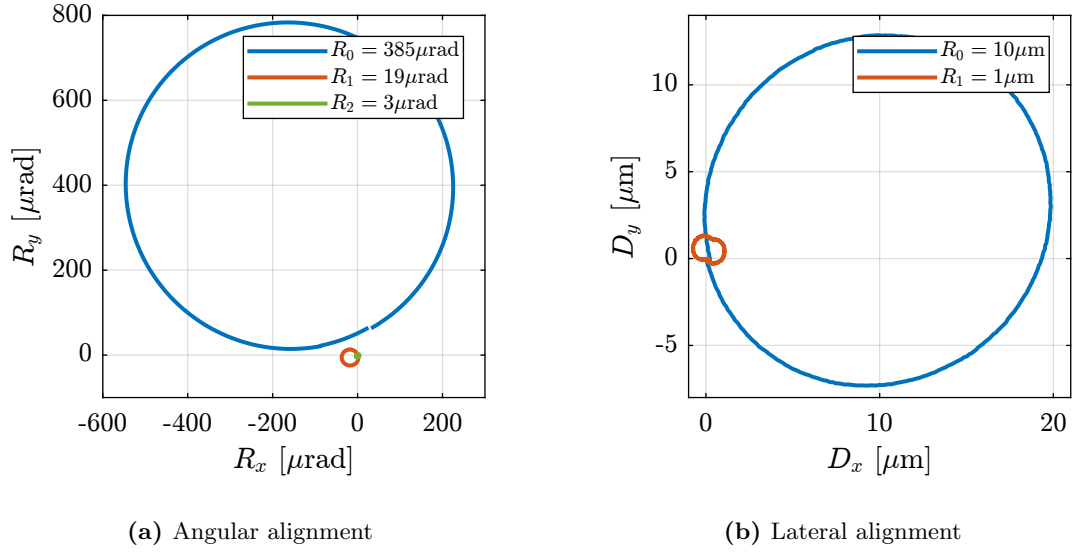


Figure 1.5: Measured angular (a) and lateral (b) errors during a full spindle rotation. Between two rotations, the micro-hexapod is adjusted to better align the two spheres with the rotation axis.

Table 1.1: Estimated measurement range for each interferometer, and for three different directions.

	D_x	D_y	D_z
d_1 (y)	1.0 mm	> 2 mm	1.35 mm
d_2 (y)	0.8 mm	> 2 mm	1.01 mm
d_3 (x)	> 2 mm	1.06 mm	1.38 mm
d_4 (x)	> 2 mm	0.99 mm	0.94 mm
d_5 (z)	1.33 mm	1.06 mm	> 2 mm

architecture, the accuracy of the metrology is not an issue. Only the bandwidth and noise characteristics of the external metrology are important. Yet, some elements effecting the accuracy of the metrology are discussed here.

First, the “metrology kinematics” (discussed in Section 1.1) is only approximate (i.e. valid for very small displacements). This can be seen when performing lateral $[D_x, D_y]$ scans using the micro-hexapod while recording the vertical interferometer (Figure 1.6a). As the interferometer is pointing to a sphere and not to a plane, lateral motion of the sphere is seen as a vertical motion by the top interferometer.

Then, the reference spheres have some deviations with respect to an ideal sphere. They are meant to be used with capacitive sensors which are integrating the shape errors over large surfaces. When using interferometers, the size of the “light spot” on the sphere surface is a circle with a diameter $\approx 50 \mu m$, therefore the system is more sensitive to shape errors with small features.

As the interferometer light is travelling in air, the measured distance is sensitive to any variation in the refractive index of the air. Therefore, any variation of air temperature, pressure or humidity will induce measurement errors. For a measurement length of $40 mm$, a temperature variation of $0.1 ^\circ C$ induces an errors in the distance measurement of $\approx 4 nm$.

Finally, even in vacuum and in the absence of target motion, the interferometers are affected by noise [1]. The effect of the noise on the translation and rotation measurements is estimated in Figure 1.6b.

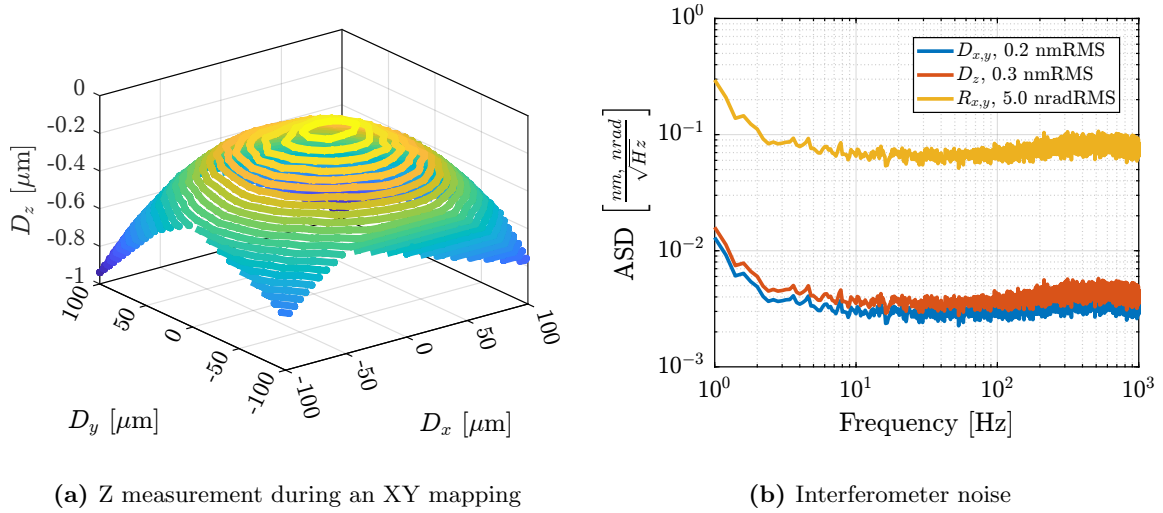


Figure 1.6: Estimated measurement errors of the metrology. Cross-coupling between lateral motion and vertical measurement is shown in (a). Effect of interferometer noise on the measured translations and rotations is shown in (b).

2 Identified Open Loop Plant

- Force sensors: $\mathbf{V}_s = [V_{s1}, V_{s2}, V_{s3}, V_{s4}, V_{s5}, V_{s6}]$
- Encoders: $\mathbf{d}_e = [d_{e1}, d_{e2}, d_{e3}, d_{e4}, d_{e5}, d_{e6}]$
- Interferometers: $\mathbf{d} = [d_1, d_2, d_3, d_4, d_5]$
- Command signal: $\mathbf{u} = [u_1, u_2, u_3, u_4, u_5, u_6]$
- Voltage across the piezoelectric stack actuator: $\mathbf{V}_a = [V_{a1}, V_{a2}, V_{a3}, V_{a4}, V_{a5}, V_{a6}]$
- Motion of the sample measured by external metrology: $\mathbf{y}_X = [D_x, D_y, D_z, R_x, R_y, R_z]$
- Error of the sample measured by external metrology: $\epsilon_{\mathcal{X}} = [\epsilon_{D_x}, \epsilon_{D_y}, \epsilon_{D_z}, \epsilon_{R_x}, \epsilon_{R_y}, \epsilon_{R_z}]$
- Error of the struts measured by external metrology: $\epsilon_{\mathcal{L}} = [\epsilon_{\mathcal{L}_1}, \epsilon_{\mathcal{L}_2}, \epsilon_{\mathcal{L}_3}, \epsilon_{\mathcal{L}_4}, \epsilon_{\mathcal{L}_5}, \epsilon_{\mathcal{L}_6}]$
- Spindle angle setpoint (or encoder): r_{R_z}
- Translation stage setpoint: r_{D_y}
- Tilt stage setpoint: r_{R_y}

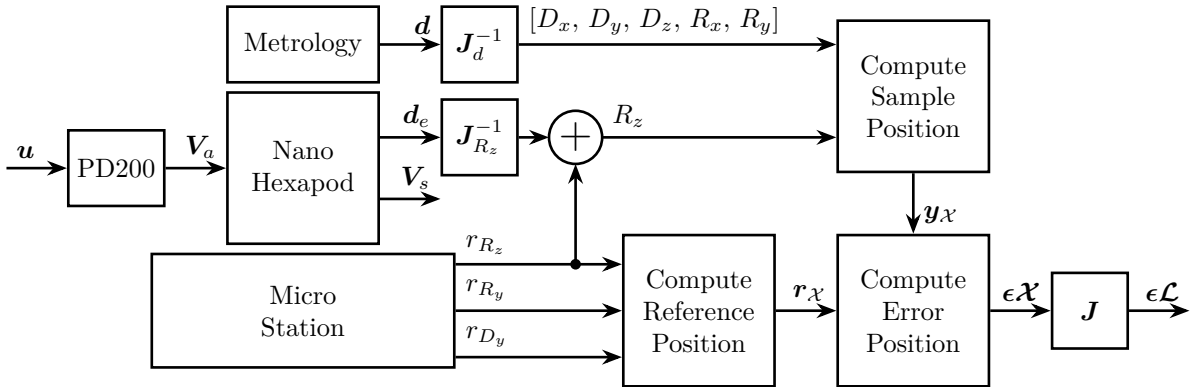


Figure 2.1: Schematic of the

2.1 First Open-Loop Plant Identification

The plant dynamics is first identified for a fixed spindle angle (at 0 deg) and without any payload. The model dynamics is also identified in the same conditions.

A first comparison between the model and the measured dynamics is done in Figure 2.2. A good match can be observed for the diagonal dynamics (except the high frequency modes which are not modeled). However, the coupling for the transfer function from command signals \mathbf{u} to estimated strut motion from the external metrology $e\mathcal{L}$ is larger than expected (Figure 2.2a).

The experimental time delay estimated from the FRF (Figure 2.2a) is larger than expected. After investigation, it was found that the additional delay was due to digital processing unit¹ that was used to read the interferometers in the Speedgoat. This issue was later solved.

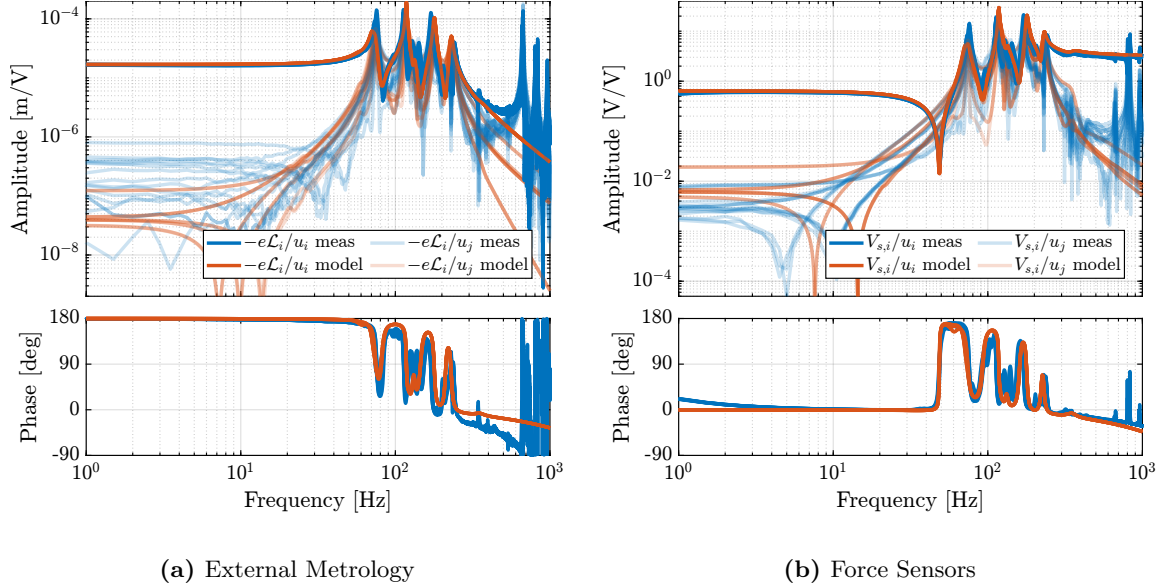


Figure 2.2: Comparison between the measured dynamics and the multi-body model dynamics. Both for the external metrology (a) and force sensors (b).

2.2 Better Angular Alignment

One possible explanation of the increased coupling observed in Figure 2.2a is the poor alignment between the external metrology axes (i.e. the interferometer supports) and the nano-hexapod axes. To estimate this alignment, a decentralized low-bandwidth feedback controller based on the nano-hexapod encoders is implemented. This allowed to perform two straight movements of the nano-hexapod along the x and y axes in the frame of the nano-hexapod. During these two movements, the external metrology measurement is recorded and shown in Figure 2.3. It was found that there is a misalignment of 2.7 degrees (rotation along the vertical axis) between the interferometer axes and nano-hexapod axes. This was corrected by adding an offset to the spindle angle. To check that the alignment has improved, the same movement was performed using the nano-hexapod while recording the signal of the external metrology. Results shown in Figure 2.3b are indeed indicating much better alignment.

¹The “PEPU” [2] was used for digital protocol conversion between the interferometers and the Speedgoat

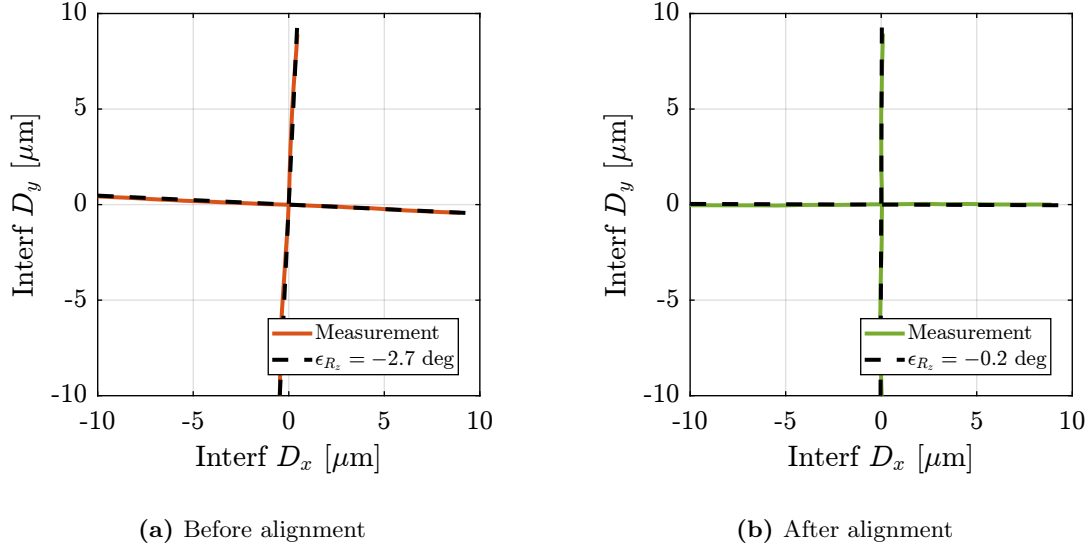


Figure 2.3: Measurement of the Nano-Hexapod axes in the frame of the external metrology. Before alignment (a) and after alignment (b).

2.3 Open-Loop Identification after alignment

The plant dynamics is identified after the fine alignment and is compared with the model dynamics in Figure 2.4. Compared to the initial identification shown in Figure 2.2a, the obtained coupling has decreased and is now close to the coupling obtained with the multi-body model. At low frequency (below 10 Hz) all the off-diagonal elements have an amplitude ≈ 100 times lower compared to the diagonal elements, indicating that a low bandwidth feedback controller can be implemented in a decentralized way (i.e. 6 SISO controllers).


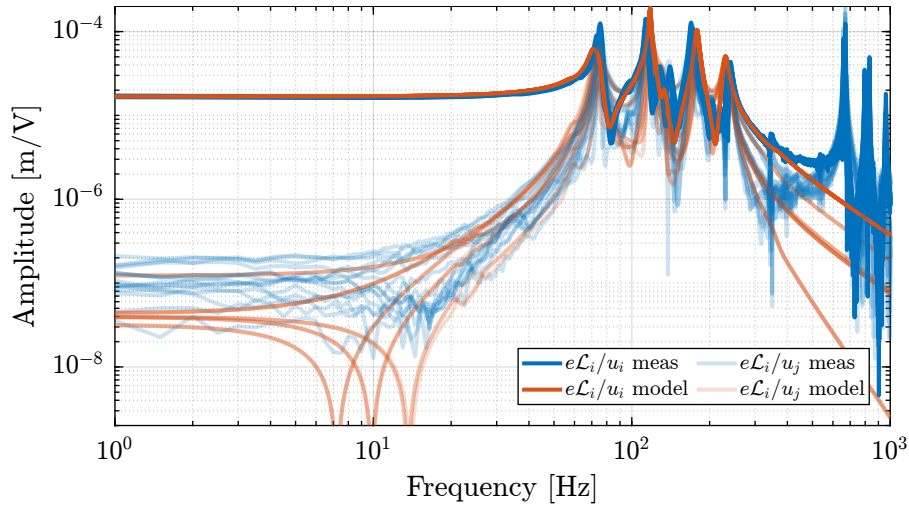


Figure 2.4: Decrease of the coupling with better R_z alignment

2.4 Effect of Payload Mass

The system dynamics was identified with four payload conditions that are shown in Figure 2.5. The obtained direct terms are compared with the model dynamics in Figure 2.6.

It is interesting to note that the anti-resonances in the force sensor plant are now appearing as minimum-phase, as the model predicts (Figure 2.6b).

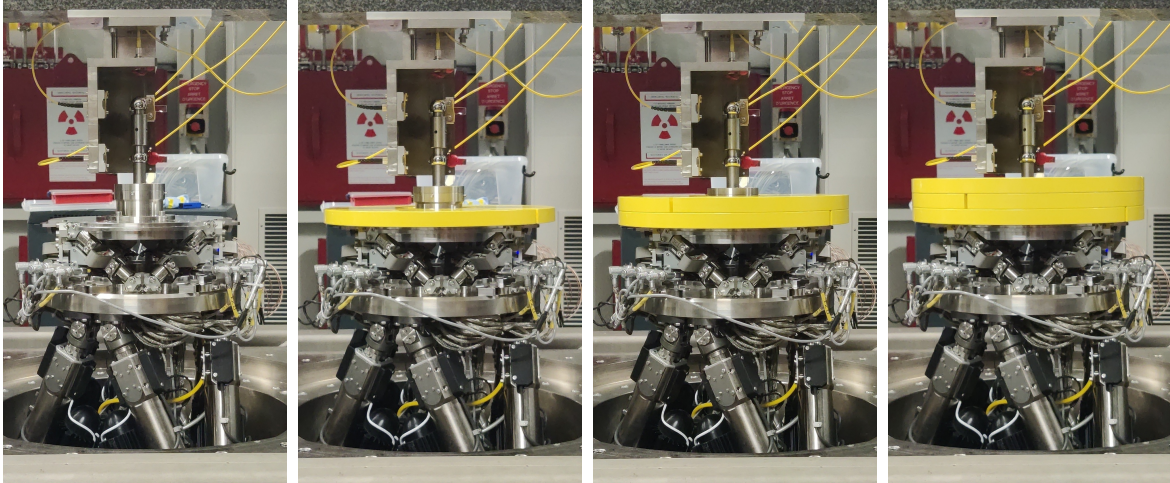

(a) $m = 0$ kg

(b) $m = 13$ kg

(c) $m = 26$ kg

(d) $m = 39$ kg

Figure 2.5: The four tested payload conditions. (a) without payload. (b) with 13 kg payload. (c) with 26 kg payload. (d) with 39 kg payload.

2.5 Effect of Spindle Rotation

The dynamics was then identified while the Spindle was rotating at constant velocity. Three identification experiments were performed: no spindle rotation, spindle rotation at 36 deg/s and at 180 deg/s.

The comparison of the obtained dynamics from command signal u to estimated strut error $e\mathcal{L}$ is done in Figure 2.7. Both direct terms (Figure 2.7a) and coupling terms (Figure 2.7b) are unaffected by the rotation. The same can be observed for the dynamics from the command signal to the encoders and to the force sensors. This confirms that the rotation has no significant effect on the plant dynamics. This also indicates that the metrology kinematics is correct and is working in real time.

2.6 Identification of Spurious modes

These are made to identify the modes of the spheres

Also discuss other observed modes

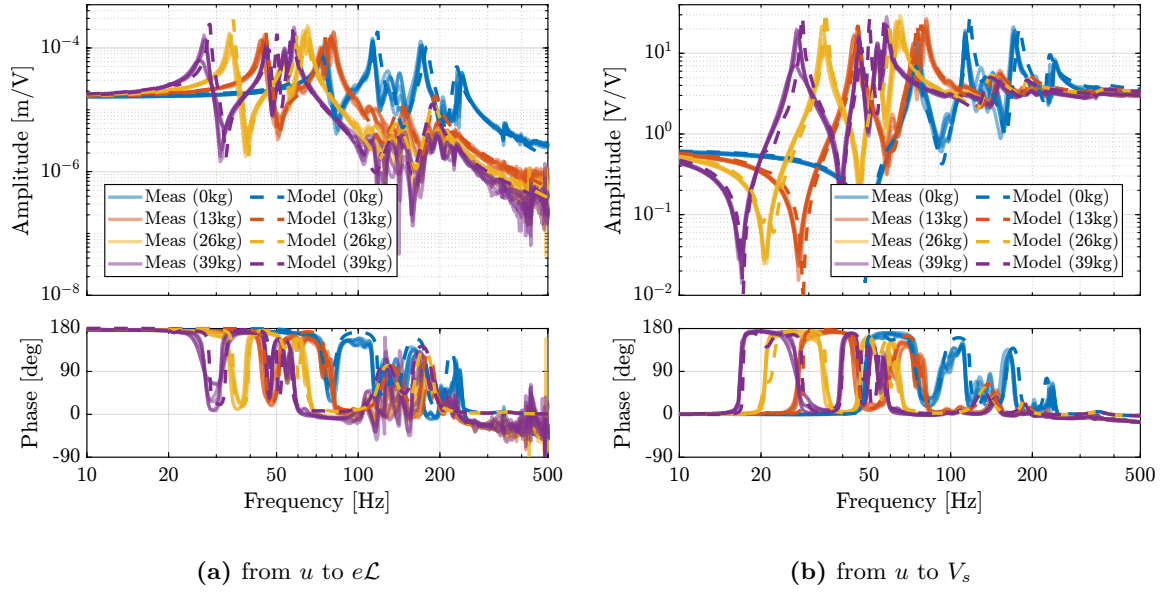


Figure 2.6: Comparison of the diagonal elements (i.e. “direct” terms) of the measured FRF matrix and the dynamics identified from the Simscape model. Both for the dynamics from u to $e\mathcal{L}$ (a) and from u to V_s (b)

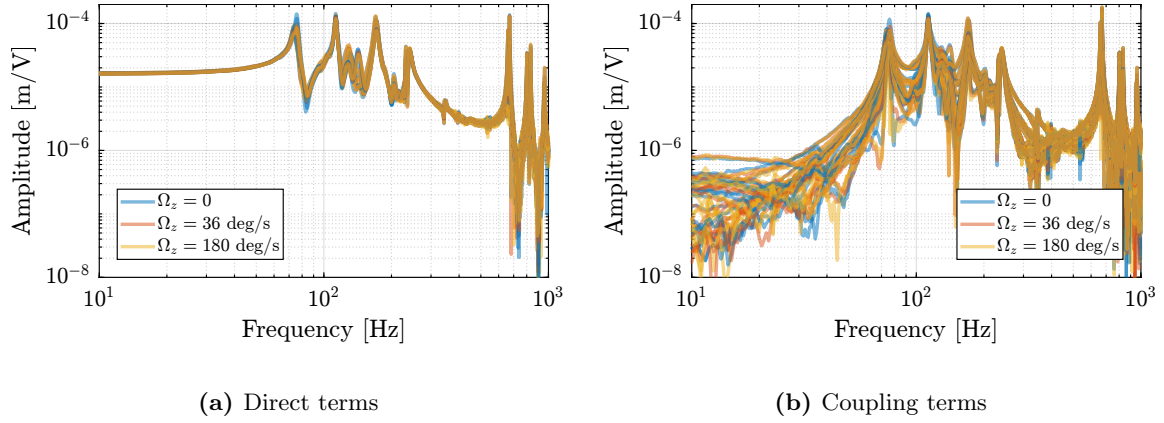


Figure 2.7: Effect of the spindle rotation on the plant dynamics from u to $e\mathcal{L}$. Three rotational velocities are tested (0 deg/s, 36 deg/s and 180 deg/s). Both direct terms (a) and coupling terms (b) are displayed.

Conclusion

Thanks to the model, poor alignment between the nano-hexapod axes and the external metrology axes could be identified. After alignment, the identified dynamics is well matching with the multi-body model.

Also, the observed effects of the payload mass and of the spindle rotation on the dynamics are well matching the model predictions.

3 Decentralized Integral Force Feedback

Before implementing a position controller, an active damping controller was first implemented as shown in Figure 3.1. It consisted of a decentralized Integral Force Feedback controller \mathbf{K}_{IFF} , with all the diagonal terms being equal (3.2).

$$\mathbf{K}_{\text{IFF}} = K_{\text{IFF}} \cdot \mathbf{I}_6 = \begin{bmatrix} K_{\text{IFF}} & & 0 \\ & \ddots & \\ 0 & & K_{\text{IFF}} \end{bmatrix} \quad (3.1)$$

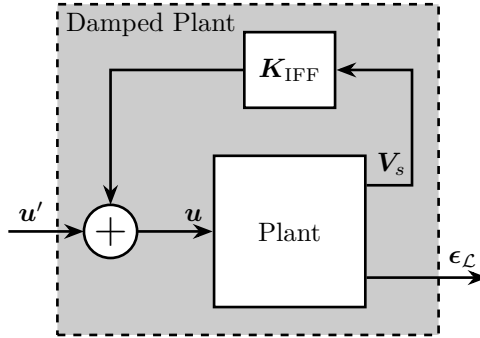


Figure 3.1: Block diagram of the implemented decentralized IFF controller. The controller \mathbf{K}_{IFF} is a diagonal controller with the same elements on every diagonal term K_{IFF} .

3.1 IFF Plant

As the multi-body model is going to be used to estimate the stability of the IFF controller and to optimize achievable damping, it is first checked if this model accurately represents the system dynamics.

In Figure 2.6b, it was shown that the model well captures the dynamics from each actuator to its collocated force sensor, as that for all considered payloads. The model is also accurate for the dynamics from an actuator to the force sensors in the other struts (i.e. the off-diagonal dynamics) as shown in Figure 3.2.

3.2 IFF Controller

A decentralized IFF controller is there designed such that it adds damping to the suspension modes of the nano-hexapod for all considered payloads. The frequency of the suspension modes are ranging from ≈ 30 Hz to ≈ 250 Hz (Figure 2.6b), and therefore the IFF controller should provide integral action in

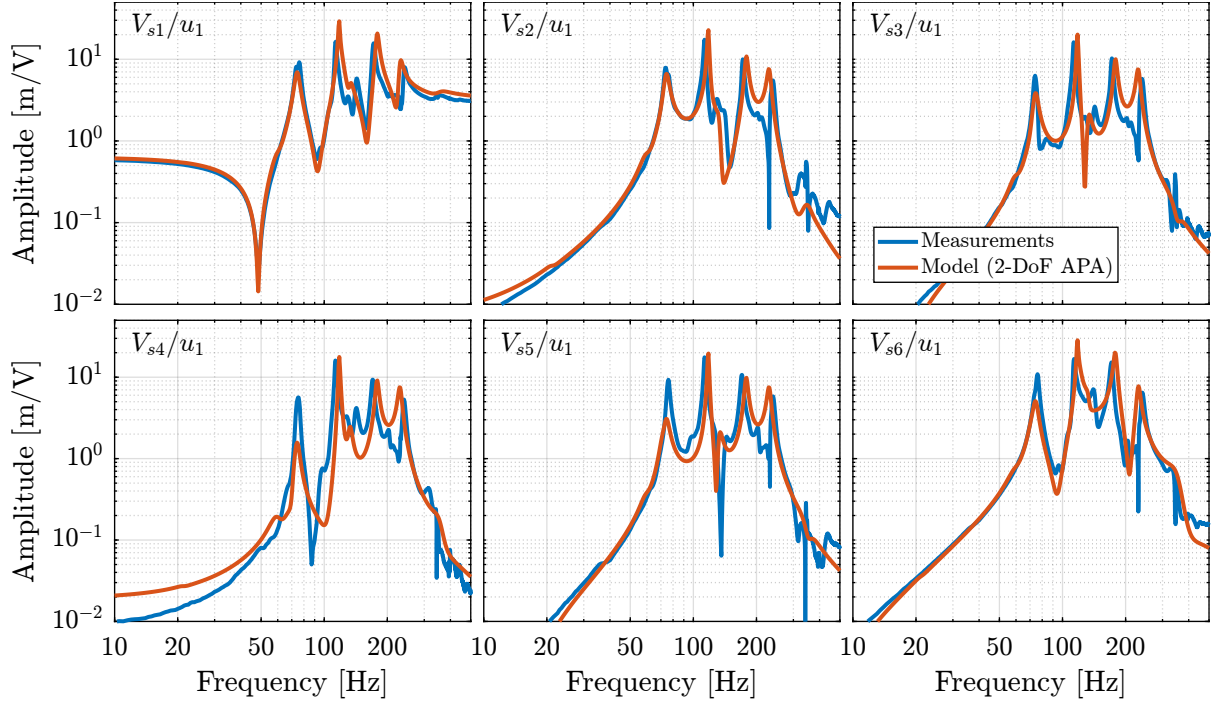



Figure 3.2: Comparison of the measured (in blue) and modeled (in red) frequency transfer functions from the first control signal u_1 to the six force sensor voltages V_{s1} to V_{s6}

this frequency range. A second order high pass filter (cut-off frequency of 10 Hz) is added to limit the low frequency gain.


The bode plot of the decentralized IFF controller is shown in Figure 3.3a and the “decentralized loop-gains” for all considered payload masses are shown in Figure 3.3b. It can be seen that the loop-gain is larger than 1 around suspension modes indicating that some damping should be added to the suspension modes.

$$K_{\text{IFF}} = g_0 \cdot \underbrace{\frac{1}{s}}_{\text{int}} \cdot \underbrace{\frac{s^2/\omega_z^2}{s^2/\omega_z^2 + 2\xi_z s/\omega_z + 1}}_{\text{2nd order LPF}}, \quad (g_0 = -100, \omega_z = 2\pi 10 \text{ rad/s}, \xi_z = 0.7) \quad (3.2)$$

To estimate the added damping, a root-locus plot is computed using the multi-body model (Figure 3.4). It can be seen that for all considered payloads, the poles are bounded to the “left-half plane” indicating that the decentralized IFF is robust. The closed-loop poles for the chosen value of the gain are displayed by black crosses. It can be seen that while damping can be added for all payloads (as compared to the open-loop case), the optimal value of the gain could be tuned separately for each payload. For instance, for low payload masses, a higher value of the IFF controller gain could lead to better damping. However, in this study, it was chosen to implement a fix (i.e. non-adaptive) decentralized IFF controller.

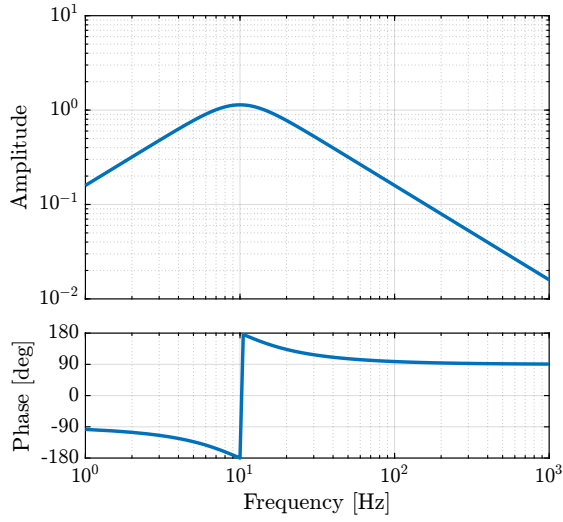


(a) Bode plot of K_{IFF}

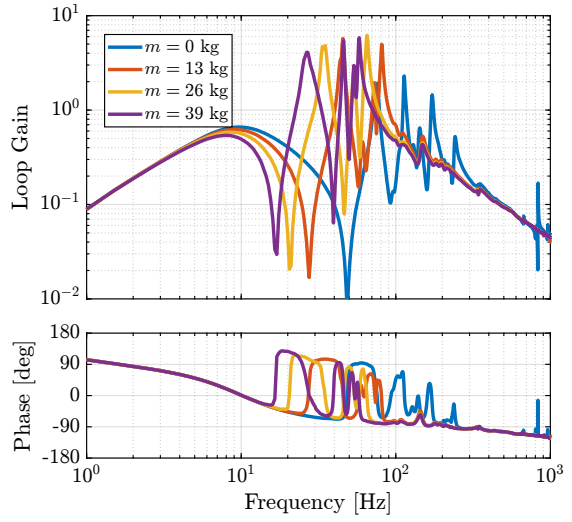

(b) Decentralized Loop gains

Figure 3.3: Bode plot of the decentralized IFF controller (a). The decentralized controller K_{IFF} multiplied by the identified dynamics from u_1 to V_{s1} for all payloads are shown in (b)

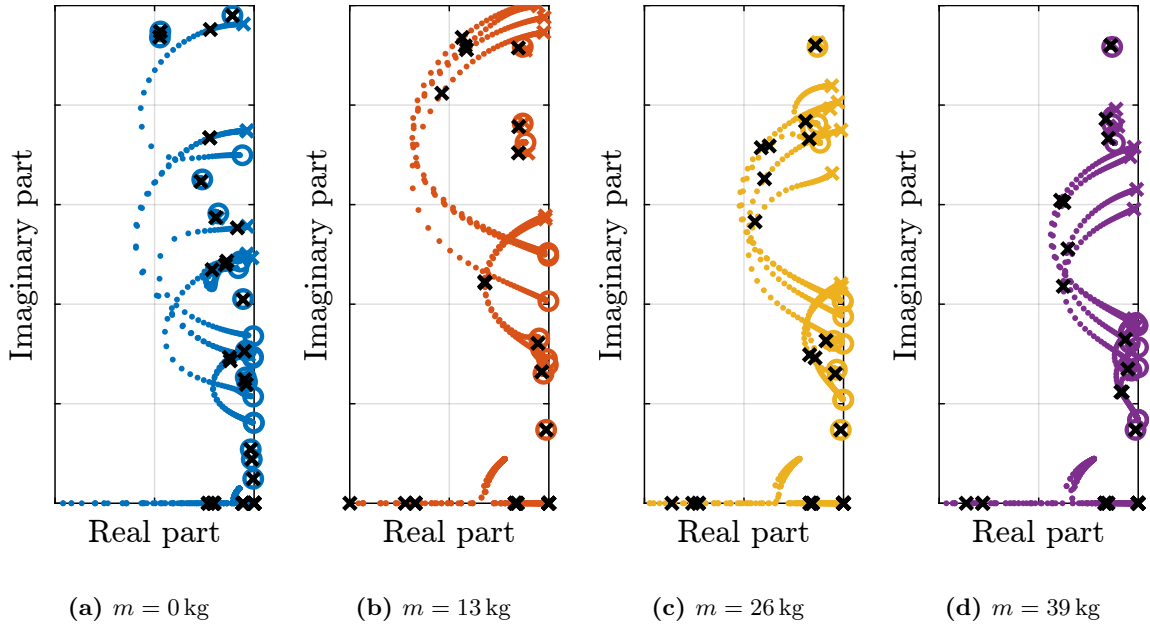

(a) $m = 0$ kg

(b) $m = 13$ kg

(c) $m = 26$ kg

(d) $m = 39$ kg

Figure 3.4: Root Locus plots for the designed decentralized IFF controller and using the multi-body model. Black crosses indicate the closed-loop poles for the chosen value of the gain.

3.3 Estimated Damped Plant

As the model is accurately modelling the system dynamics, it can be used to estimate the damped plant, i.e. the transfer functions from \mathbf{u}' to \mathcal{L} . The obtained damped plants are compared with the open-loop plants in Figure 3.5. The peak amplitudes corresponding to the suspension modes are approximately reduced by a factor 10 for all considered payloads, and with the same decentralized IFF controller.

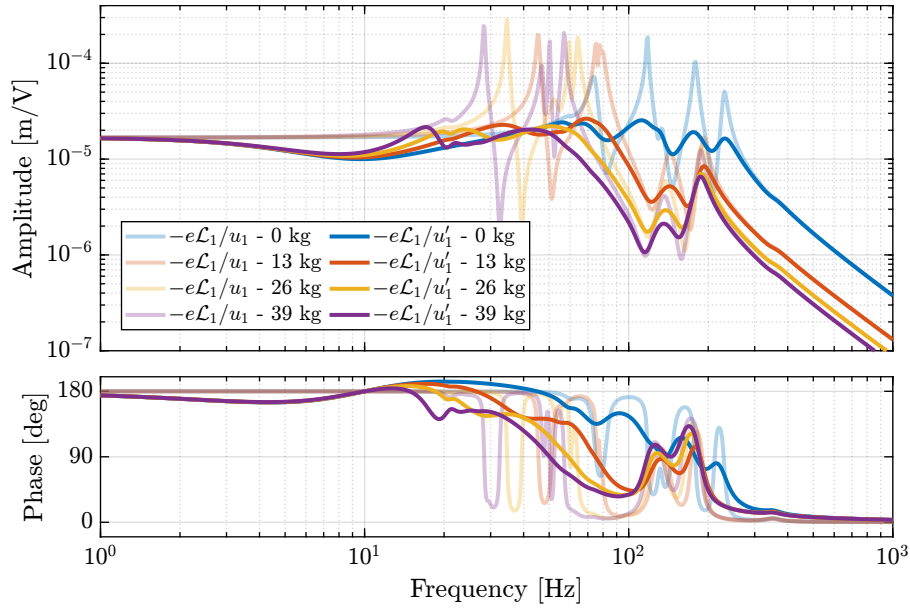


Figure 3.5: Comparison of the open-loop plants and the estimated damped plant with Decentralized IFF.

Conclusion

4 High Authority Control in the frame of the struts

The position of the sample is actively stabilized by implementing a High-Authority-Controller as shown in Figure 4.1.

$$\mathbf{K}_{\text{HAC}} = K_{\text{HAC}} \cdot \mathbf{I}_6 = \begin{bmatrix} K_{\text{HAC}} & & 0 \\ & \ddots & \\ 0 & & K_{\text{HAC}} \end{bmatrix} \quad (4.1)$$

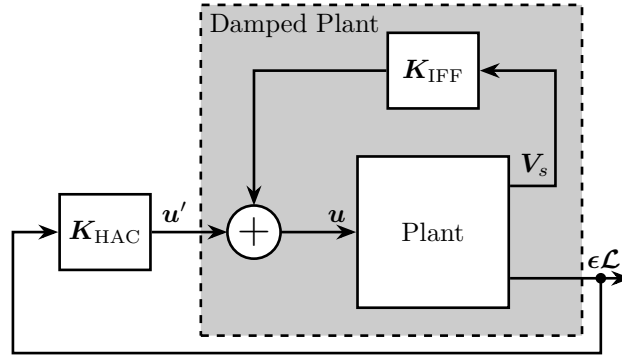


Figure 4.1: Block diagram of the implemented HAC-IFF controllers. The controller \mathbf{K}_{HAC} is a diagonal controller with the same elements on every diagonal term K_{HAC} .

4.1 Damped Plant

The damped plants (i.e. the transfer function from \mathbf{u}' to $\epsilon\mathcal{L}$) were identified for all payload conditions. To verify if the model accurately represents the damped plants, both direct terms and coupling terms corresponding to the first actuator are compared in Figure 4.2.

The six direct terms for all four payload conditions are compared with the model in Figure 4.3a. It is shown that the model accurately represents the dynamics for all payloads.

In Section 4, a High Authority Controller is tuned to be robust to the change of dynamics due to different payloads used. Without decentralized IFF being applied, the controller would have had to be robust to all the undamped dynamics shown in Figure 4.3b, which is a very complex control problem. With the applied decentralized IFF, the HAC instead had to be robust to all the damped dynamics shown in Figure 4.3b, which is easier from a control perspective. This is one of the key benefit of using the HAC-LAC strategy.


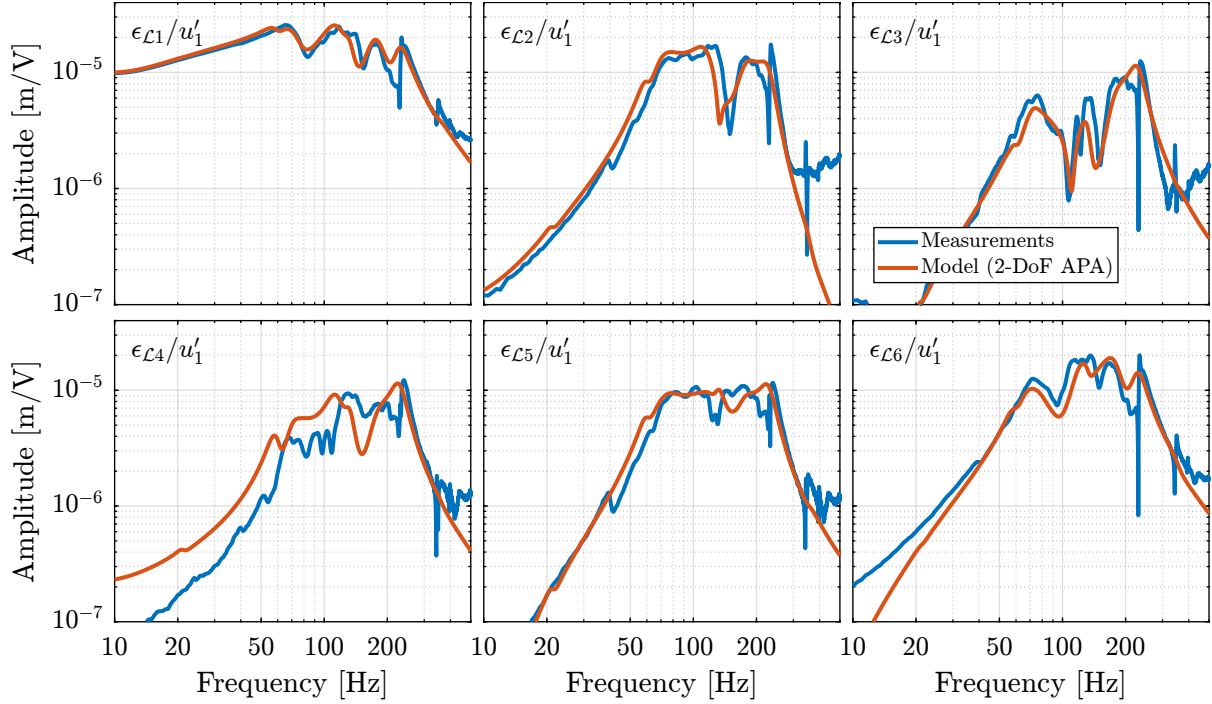


Figure 4.2: Comparison of the measured (in blue) and modeled (in red) frequency transfer functions from the first control signal (u'_1) of the damped plant to the estimated errors ($\epsilon_{\mathcal{L}_i}$) in the frame of the six struts by the external metrology

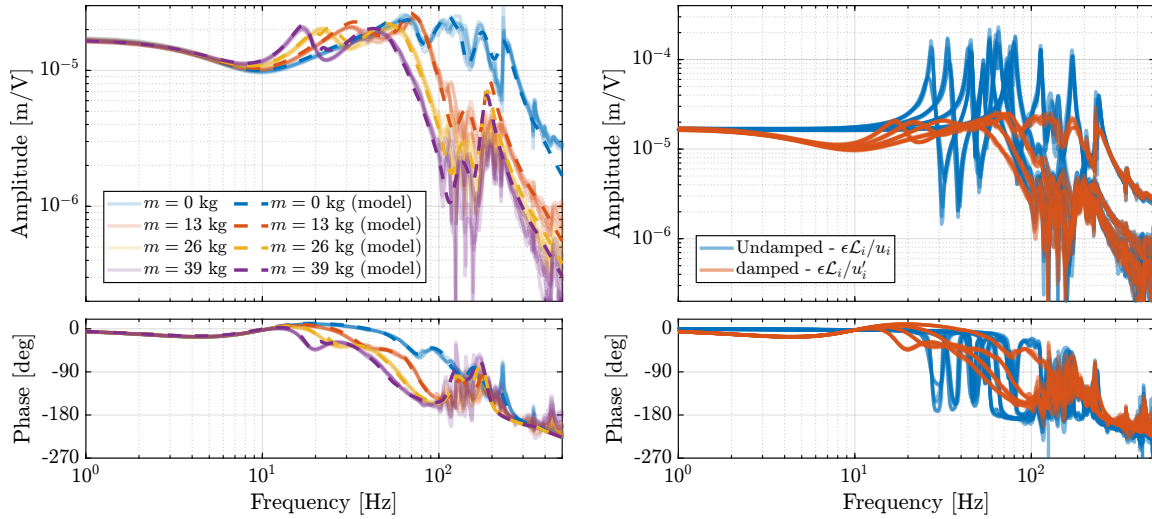

(a) Effect of payload mass on $\epsilon_{\mathcal{L}_i}/u'_i$

(b) Undamped and damped plants

Figure 4.3: Comparison of the measured damped plants and modeled plants for all considered payloads, only “direct” terms ($\epsilon_{\mathcal{L}_i}/u'_i$) are displayed (a). Comparison of all undamped $\epsilon_{\mathcal{L}_i}/u'_i$ and damped $\epsilon_{\mathcal{L}_i}/u'_i$ measured frequency response functions for all payloads is done in (b).

4.2 Robust Controller Design

A first diagonal controller was designed to be robust to change of payloads, which means that every damped plants shown in Figure 4.3b should be considered during the controller design. For a first design, a crossover frequency of 5 Hz for chosen. One integrator is added to increase the low frequency gain, a lead is added around 5 Hz to increase the stability margins and a first order low pass filter with a cut-off frequency of 30 Hz is added to improve the robustness to dynamical uncertainty at high frequency. The obtained “decentralized” loop-gains are shown in Figure 4.4a.

$$K_{\text{HAC}} = g_0 \cdot \underbrace{\frac{\omega_c}{s}}_{\text{int}} \cdot \underbrace{\frac{1}{\sqrt{\alpha}} \frac{1 + \frac{s}{\omega_c/\sqrt{\alpha}}}{1 + \frac{s}{\omega_c\sqrt{\alpha}}}}_{\text{lead}} \cdot \underbrace{\frac{1}{1 + \frac{s}{\omega_0}}}_{\text{LPF}}, \quad (\omega_c = 2\pi 5 \text{ rad/s}, \alpha = 2, \omega_0 = 2\pi 30 \text{ rad/s}) \quad (4.2)$$

The closed-loop stability is verified by computing the characteristic Loci (Figure 4.4b).


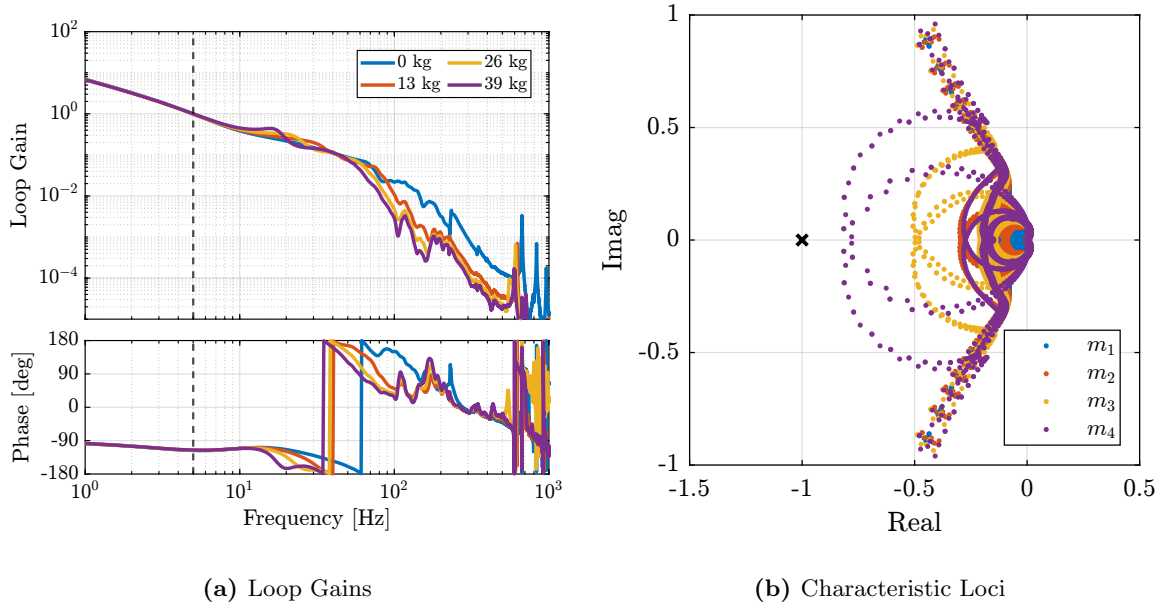


Figure 4.4: Robust High Authority Controller. “Decentralized loop-gains” are shown in (a) and characteristic loci are shown in (b)


4.3 Estimation of performances

To estimate the performances that can be expected with this HAC-LAC architecture and the designed controllers, two simulations of tomography experiments were performed¹. The rotational velocity was set to 30rpm, and no payload was added on top of the nano-hexapod. An open-loop simulation and a closed-loop simulation were performed and compared in Figure 4.5.

¹Note that the eccentricity of the “point of interest” with respect to the Spindle rotation axis has been tuned from the measurements.

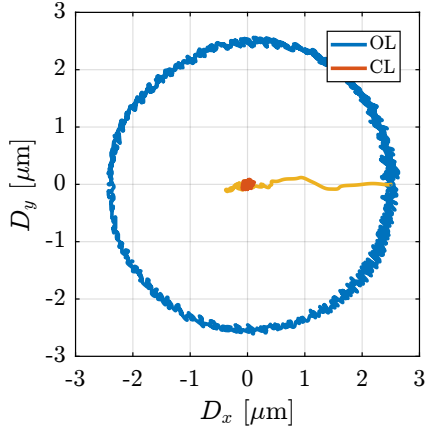


(a) XY plane

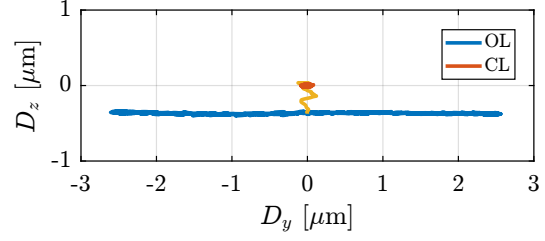


(b) YZ plane

Figure 4.5: Position error of the sample in the XY (a) and YZ (b) planes during a simulation of a tomography experiment at 30RPM. No payload is placed on top of the nano-hexapod.

Then the same tomography experiment (i.e. constant spindle rotation at 30rpm, and no payload) was performed experimentally. The measured position of the “point of interest” during the experiment are shown in Figure 4.6.

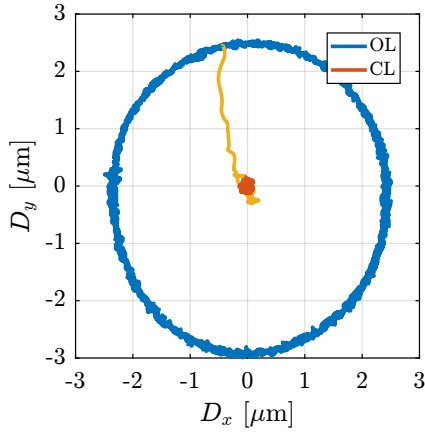

(a) XY plane

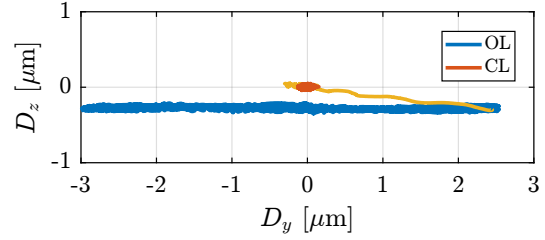

(b) YZ plane

Figure 4.6: Experimental results of a tomography experiment at 30RPM without payload. Position error of the sample is shown in the XY (a) and YZ (b) planes.

Even though the simulation (Figure 4.5) and the experimental results (Figure 4.6) are looking similar, the most important metric to compare is the RMS values of the positioning errors in closed-loop. These are computed for both the simulation and the experimental results and are compared in Table 4.1. The lateral and vertical errors are similar, however the tilt (R_y) errors are underestimated by the model, which is reasonable as disturbances in R_y were not modeled.

Results obtained with this conservative HAC are already close to the specifications.

Table 4.1: RMS values of the errors for a tomography experiment at 30RPM and without payload. Experimental results and simulation are compared.

	D_y	D_z	R_y
Experiment (OL)	1.8 μmRMS	24 nmRMS	10 μradRMS
Simulation (CL)	30 nmRMS	8 nmRMS	73 nradRMS
Experiment (CL)	39 nmRMS	11 nmRMS	130 nradRMS
Specifications (CL)	30 nmRMS	15 nmRMS	250 nradRMS

4.4 Robustness to change of payload

To verify the robustness to the change of payload mass, four simulations of tomography experiments were performed with payloads as shown Figure 2.5 (i.e. 0 kg, 13 kg, 26 kg and 39 kg). This time, the rotational velocity was set at 1rpm (i.e. 6deg/s), as it is the typical rotational velocity for heavy samples. The closed-loop systems were stable for all payload conditions, indicating good control robustness.

The tomography experiments that were simulated were then experimentally conducted. For each payload, a spindle rotating was first performed in open-loop, and then the loop was closed during another full spindle rotation. An example with the 26 kg payload is shown in Figure 4.7a. The eccentricity between the “point of interest” and the spindle rotation axis is quite large as the added payload mass statically deforms the micro-station stages. To estimate the open-loop errors, it is supposed that the “point of interest” can be perfectly aligned with the spindle rotation axis. Therefore, the eccentricity is first estimated by performing a circular fit (dashed black circle in Figure 4.7a), and then subtracted from the data in Figure 4.7b. This underestimate the real condition open-loop errors as it is difficult to obtain a perfect alignment in practice.

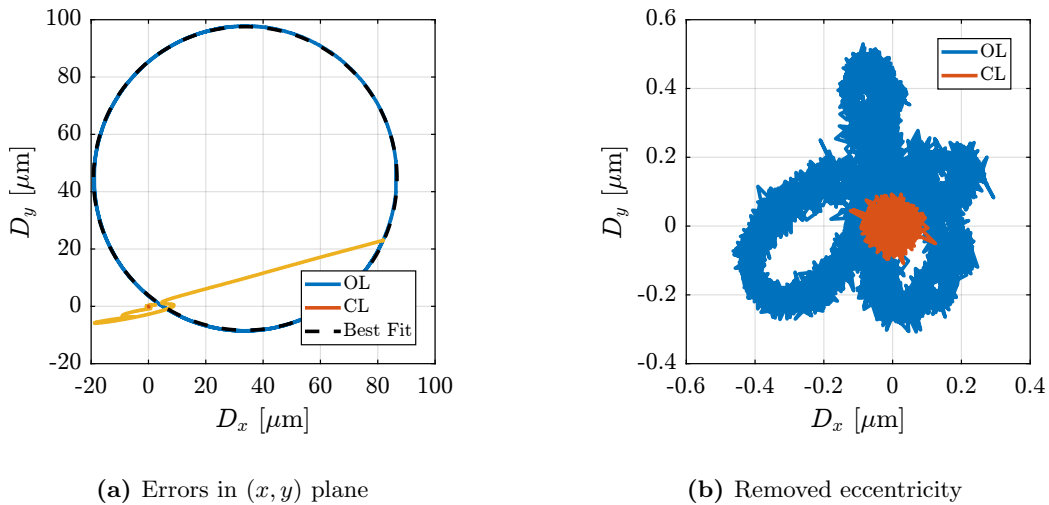


Figure 4.7: Tomography experiment with rotation velocity of 1rpm, and payload mass of 26kg. Errors in the (x, y) plane are shown in (a). The estimated eccentricity is displayed by the black dashed circle. Errors with subtracted eccentricity are shown in (b).

The RMS values of the open-loop and closed-loop errors for all masses are summarized in Table 4.2. The obtained closed-loop errors are fulfilling the requirements, except for the 39 kg payload in the lateral (D_y) direction.

Table 4.2: RMS values of the measured errors during open-loop and closed-loop tomography scans (1rpm) for all considered payloads.

	D_y	D_z	R_y
0 kg OL	142 nm RMS	32 nm RMS	460 nrad RMS
0 kg CL	15 nm RMS	5 nm RMS	55 nrad RMS
13 kg OL	149 nm RMS	26 nm RMS	470 nrad RMS
13 kg CL	25 nm RMS	6 nm RMS	55 nrad RMS
26 kg OL	202 nm RMS	36 nm RMS	1700 nrad RMS
26 kg CL	25 nm RMS	7 nm RMS	103 nrad RMS
39 kg OL	297 nm RMS	38 nm RMS	1700 nrad RMS
39 kg CL	53 nm RMS	9 nm RMS	169 nrad RMS
Specifications	30 nmRMS	15 nmRMS	250 nradRMS

Conclusion

Bibliography

- [1] J. Watchi, S. Cooper, B. Ding, C. M. Mow-Lowry, and C. Collette, “A review of compact interferometers,” *CoRR*, 2018. eprint: [1808.04175](#) (cit. on p. 9).
- [2] R. Hino, P. Fajardo, N. Janvier, T. L. Caër, and F. L. Mentec, “A position encoder processing unit,” *Proceedings of the 16th Int. Conf. on Accelerator and Large Experimental Control Systems*, vol. ICALEPCS2017, no. nil, Spain, 2018.